




**Boston
Scientific**
Advancing science for life™


 | **Staying connected**

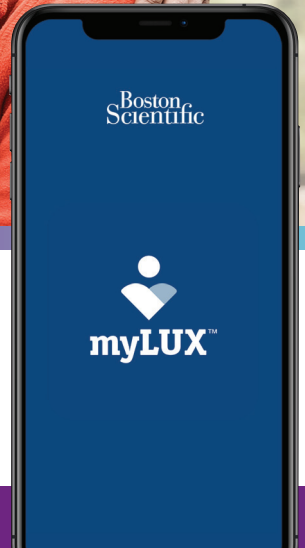

Your myLUX™ Patient App* transmits heart rhythm data stored on your LUX-Dx™ insertable cardiac monitor (ICM) device** to your clinic. It is very important to keep your app connected so your health care provider can monitor your heart rhythm remotely. **Be sure to always follow these best practices.**


*The downloadable myLUX Patient App is only available for LUX-Dx II+™ ICM. It is not available for the LUX-Dx ICM.

**References to “LUX-Dx ICM” include LUX-Dx, and LUX-Dx II+ ICM Systems.



1

Keep your smartphone charged, powered on, and connected to the internet via cellular signal or WiFi connection.



2

Keep Bluetooth® on so your app can connect to your ICM device.



3

Keep your smartphone within 6 feet (2 meters) of you while you're sleeping at night.




4


If you see a red screen and the exclamation point icon, your app is not connected. Tap **Check your connection**. Then follow the on-screen instructions.

A green screen appears when your app is successfully reconnected. Tap **Exit**.

iPhone

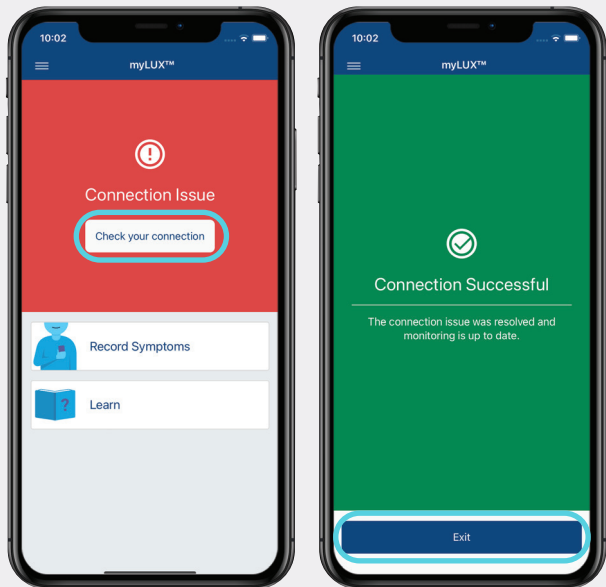

Android

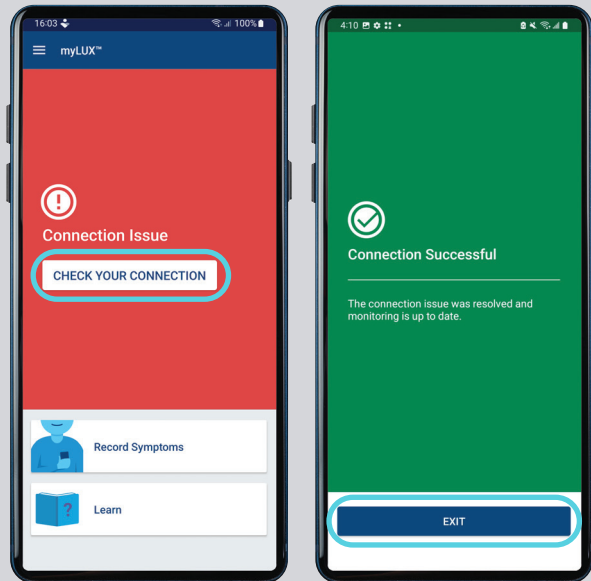


Some pictures of phone screens may look different from the screen on your mobile device, based on specific phone models or OS versions.




5

Open your myLUX™ app every once in a while. Always look for a blue screen and a check mark icon after you open your app. This confirms that your monitoring is up to date. No further action is needed from you.

iPhone

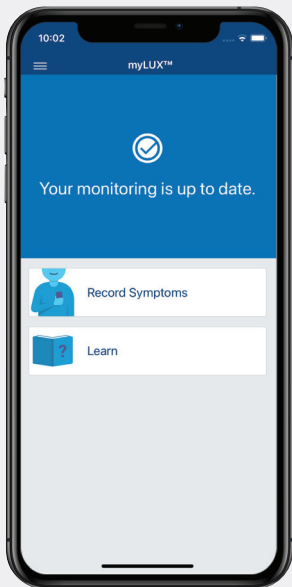

Android

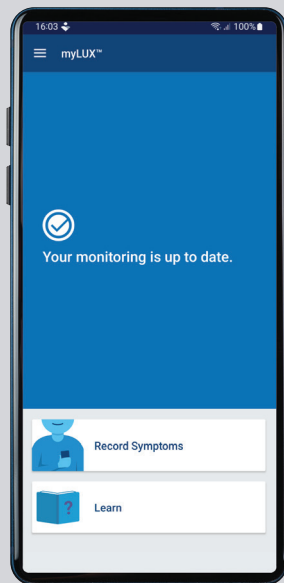


Some pictures of phone screens may look different from the screen on your mobile device, based on specific phone models or OS versions.



6


If you are using your own smartphone, remember these important things:

- **Do not quit** (i.e., do not swipe up to close the app) or **uninstall the app**
- **If you restart your smartphone**, be sure to tap the app icon to **reopen** it

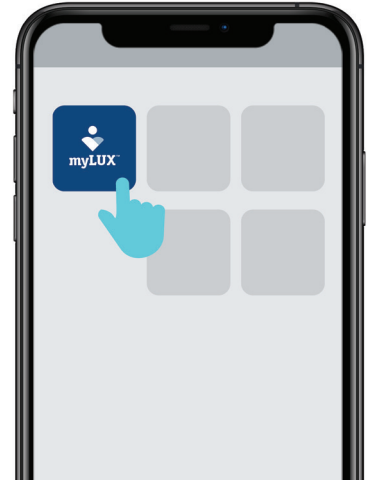


- Keep notifications turned on for your myLUX™ app

iPhone

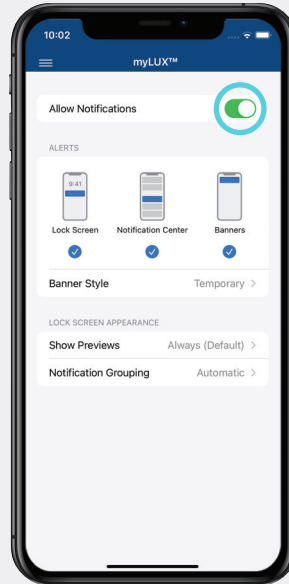


Android

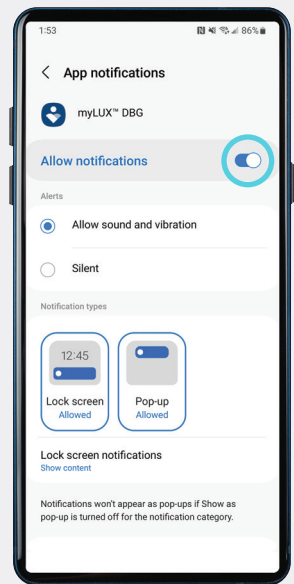


- Keep background refresh and background data usage on

iPhone

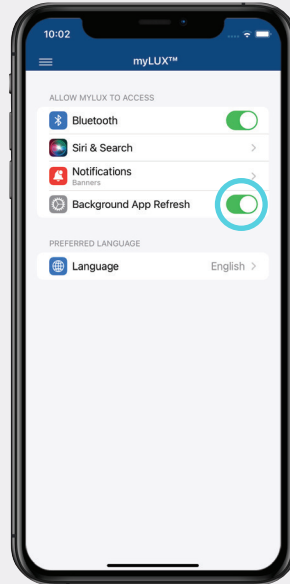


Android

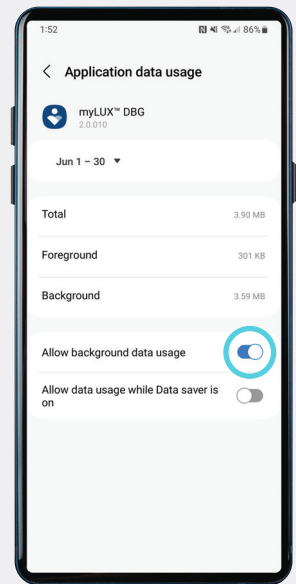

- Disable features that reduce the ability of the app to perform device checks in the background (e.g., power saving, low power, battery optimization, etc.)

iPhone

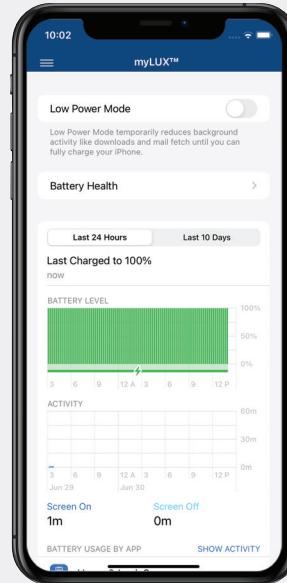

Android



To learn more about the myLUX™ app, scan this QR code to visit the myLUX™ patient website.

Need help?

Call Boston Scientific LUX-Dx™ Patient Services,
Monday–Friday during business hours,
at Australia: (+61) 1800 528 488 / New Zealand: (+64) 0508 200 886

If you need immediate medical attention, call your health care provider or seek emergency medical services.



CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings, and instructions for use can be found in the product labelling supplied with each device or at www.IFU-BSCI.com. Products shown for INFORMATION purposes only and may not be approved or for sale in certain countries.

2025 Copyright © Boston Scientific Corporation or its affiliates. All rights reserved.

All trademarks are the property of their respective owners.

Boston Scientific Pty Ltd | PO Box 332 Botany NSW 1455 Australia | Tel +61 2 8063 8100
Boston Scientific NZ Ltd, 3 Diamond Street, Eden Terrace, Auckland 1021, New Zealand

CRM-2157402-AB