



myLUX™ Patient App Step-by-step Setup Guide

Setting up your app to use with your
LUX-Dx™ ICM System

LUX-Dx ICM System Refers to LUX-Dx, and LUX-Dx II+ ICM Systems.

The downloadable myLUX Patient App is only available for LUX-Dx II+ICM. It is not available for the LUX-Dx ICM.



Already set up the myLUX™ app?

Feel free to skip this guide for now. Keep it, though, in case you get a new smartphone in the future.

If you've received an insertable cardiac monitor (ICM), you've taken a big step toward monitoring your heart for arrhythmias.

Now it's time to take the next step, setting up the myLUX™ app. Your health care provider may have given you two choices:

- If you will use your smartphone, turn to the section starting on **pages 4–5**
- If you have a mobile device provided by Boston Scientific, turn to the section starting on **pages 16–17**

IMPORTANT: To enable your ICM to check for arrhythmias, it's critical to complete the myLUX Patient App setup.

Items you'll need

1

Your smartphone

This guide will show steps for both iPhone™ and Android™ smartphones. Follow along with the column that matches your device.

Some pictures of phone screens may look different from the screen on your mobile device, based on specific phone models or OS versions.



2

Your App Store ID and password

3

The magnet provided in your myLUX™ Patient Kit box



Phone settings

1

Make sure your smartphone is turned on and you have a cellular signal or WiFi connection



2

Make sure Bluetooth® is turned on

iPhone™



Android™

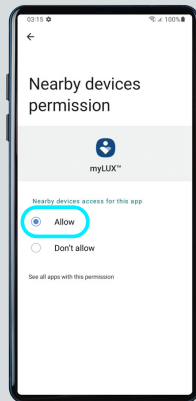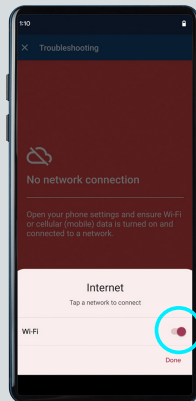

Downloading the myLUX™ app

You have two options for finding the app and downloading it:

Option 1

Scan this QR code using your smartphone. This should take you directly to the myLUX app on the App Store for an iPhone™ or on Google Play for an Android™ smartphone.


Option 2

Open the App Store if you have an iPhone or open Google Play if you have an Android smartphone. Search for the myLUX Patient App and then install it.




IMPORTANT: If you can't find the **Get** or **Install** button when downloading myLUX on your iPhone or Android device, update your operating system. If the buttons are still not visible, your device or OS version may not be compatible.

iPhone™

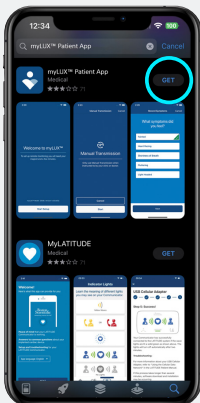

Android™

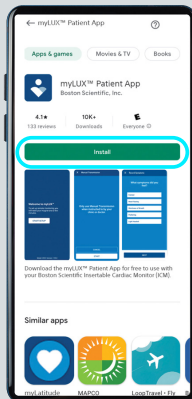

App Store



Google Play


App setup

1


After the myLUX™ app has downloaded, tap the app icon to open the app



iPhone™


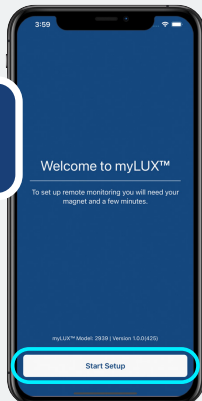


Android™

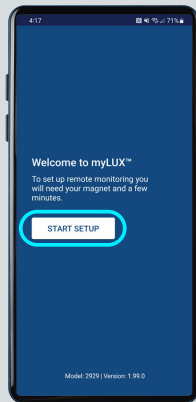

2

Tap **Start Setup**

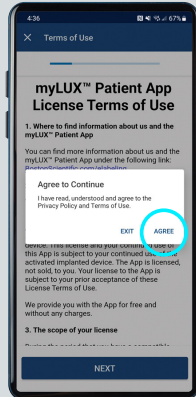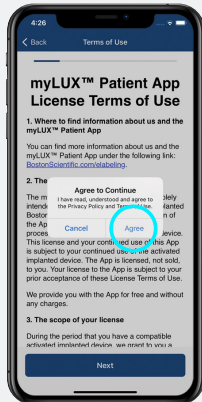

3

Read the license terms of use and privacy policy. Tap **Agree**



4

Enter your birth date



5

Tap **Allow** for notifications. You must do this so the app can send you alerts if you lose connectivity or there's other important information to know

iPhone™

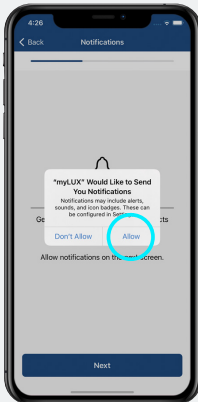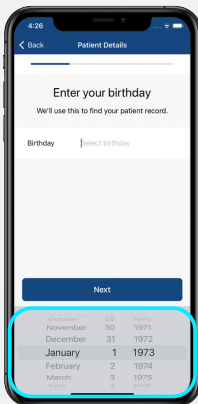


Android™

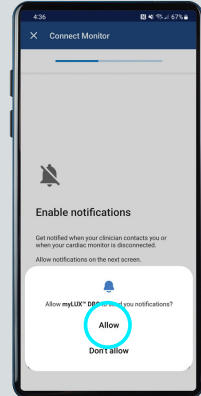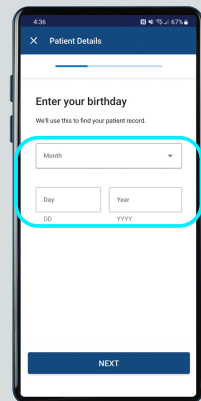


6

Tap **OK** if you have an iPhone™ to let the myLUX™ app use Bluetooth®, or tap **Allow** if you have an Android™ smartphone to allow access to nearby devices. This is required for the app to connect with your ICM

iPhone

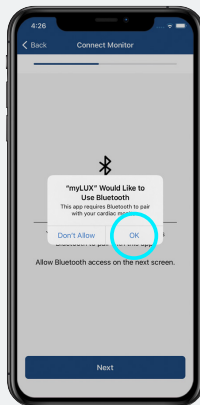

Android

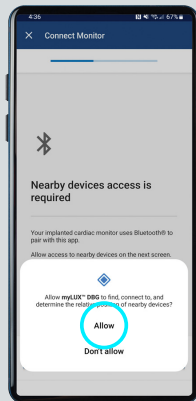



The magnet provided in your myLUX™ Patient Kit helps your myLUX app connect to your ICM device. It is also used to set up your app.

- **If you were not asked to record symptoms**, keep the magnet in a place it can easily be found
- **If you have been asked by your health care provider to use the magnet to record symptoms**, you can carry the magnet with you throughout the day
- **To avoid draining your ICM battery**, DO NOT carry the magnet in a shirt or jacket pocket over your implanted device


For information on the care and handling of the magnet, refer to the *Instructions for Use* provided with the magnet.

Complete app setup by following steps 7 through 9 on **pages 12-14**.


7

Remove the blue magnet from your myLUX™ Patient Kit. Hold the magnet over your cardiac monitor and wait for a vibration. After you feel the vibration, tap **Pair** and then move the magnet away from your chest. You may see multiple pairing requests throughout the setup process – tap **Pair** each time it comes up. This may take a couple of minutes

iPhone™

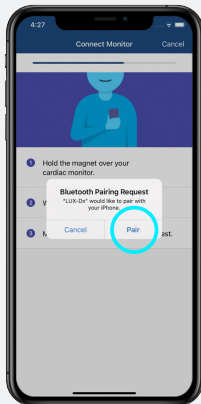


Android™

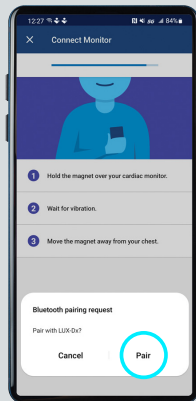


8

Enter your smartphone number or email address. Tap **Next** and you'll receive a one-time security code for verification. If it doesn't autofill, type in the code

iPhone™

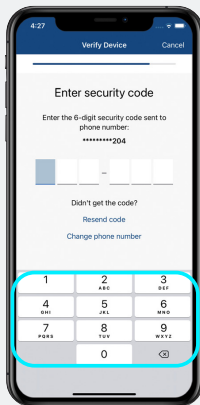

Android™

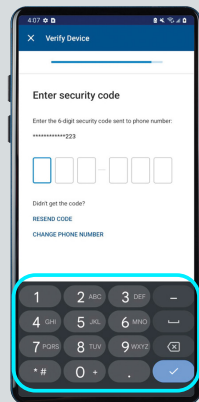



9

If you see a green screen, your setup was a success. Tap **Done**. Your myLUX™ app is now connected and can transmit data to your health care team



Additional resources

To learn more about the myLUX app, tap the **Learn** button within the app

iPhone™

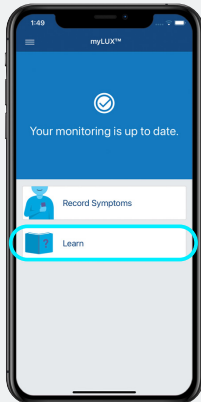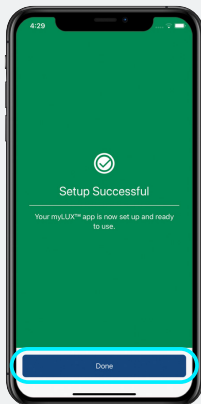

Android™

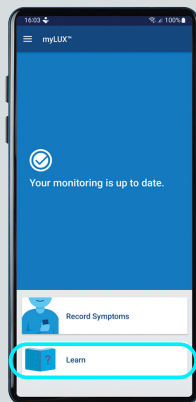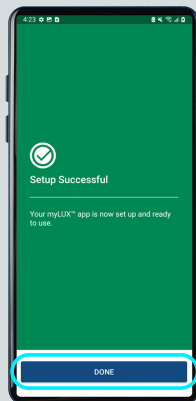



Items you'll need

1

Your Boston Scientific
provided mobile device

2

The magnet provided in
your myLUX™ Patient Kit box



The mobile device will already have the myLUX™ app pre-installed


To set up the myLUX app, follow these steps.

1

Attach the magnet to the back of your mobile device

2


Make sure you have a cellular signal or WiFi connection. Then tap **Start Setup**

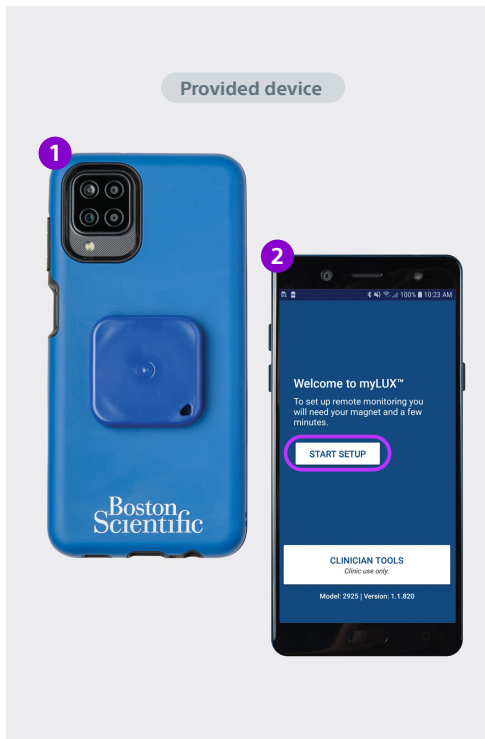

3


You'll have the opportunity to change the language.
If it's already set to the language you want, simply tap **Next**

Provided device

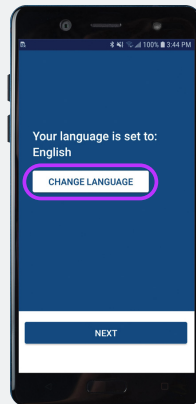

4

Read the license terms of use and privacy policy.
Tap **Agree**

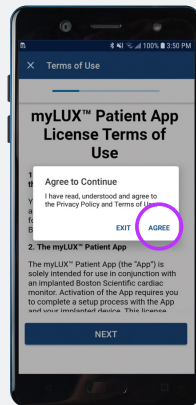



5

Enter your birth date and tap **Next**

6

Hold your mobile device over your cardiac monitor and wait for a vibration. It should take just a couple of minutes. After you feel the vibration, you can move the mobile device away from your chest. Tap **OK**

Provided device

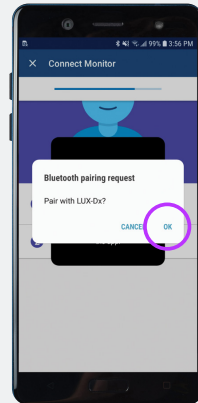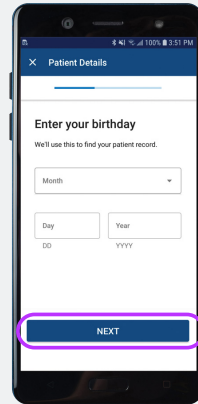



7

If you see a green screen, your setup was a success. Tap **Done**. Your myLUX™ app is now connected and can transmit data to your health care team

Additional resources

To learn more about the myLUX app, tap the **Learn** button within the app.

Provided device

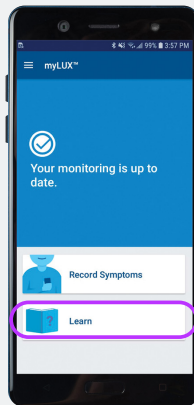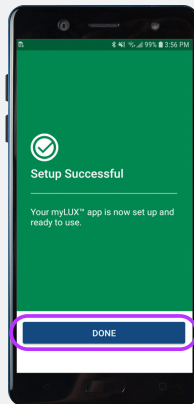





Important things to remember

Once you've completed the setup process, the LUX-Dx™ ICM System can begin monitoring your heart for arrhythmias.

Do you need help or want to contact us?

For additional help please contact the LUX-Dx™ Patient Support
Mon-Fri 9:00 to 17:30

Australia: (+61) 1800 528 488 / New Zealand: (+64) 0508 200 886

To ensure your clinic has the most up-to-date information needed to monitor your heart rhythm, it is very important to:



Keep your smartphone charged and powered on



Have a cellular signal or WiFi connection for the smartphone to work



Keep your smartphone within 2 meters of you as much as possible



Don't quit the myLUX™ app. Keep your app running in the background and be sure to reopen the app every time you restart your smartphone

CAUTION: The law restricts these devices to sale by or on the order of a physician. Indications, contraindications, warnings, and instructions for use can be found in the product labelling supplied with each device or at www.IFU-BSCI.com. Products shown for INFORMATION purposes only and may not be approved or for sale in certain countries.

Australia and New Zealand: Boston Scientific Pty Ltd | PO Box 332 Botany NSW 1455 Australia

**Boston
Scientific**

Advancing science for life™

© 2025 Boston Scientific
Corporation or its affiliates.
All rights reserved.

CRM-2157701-AA